


# A CLEAR SHOT AT BEATING YOUR DRUG TEST



## Ameritech Diagnostics Lab vs. Standard Lab Tests

The new science of specimen validity testing that takes the mask off masking agents. Give us a call at 919.243.1831 or email [sales@ameritechdiagnostics.com](mailto:sales@ameritechdiagnostics.com) to trial our next generation specimen validity testing today.










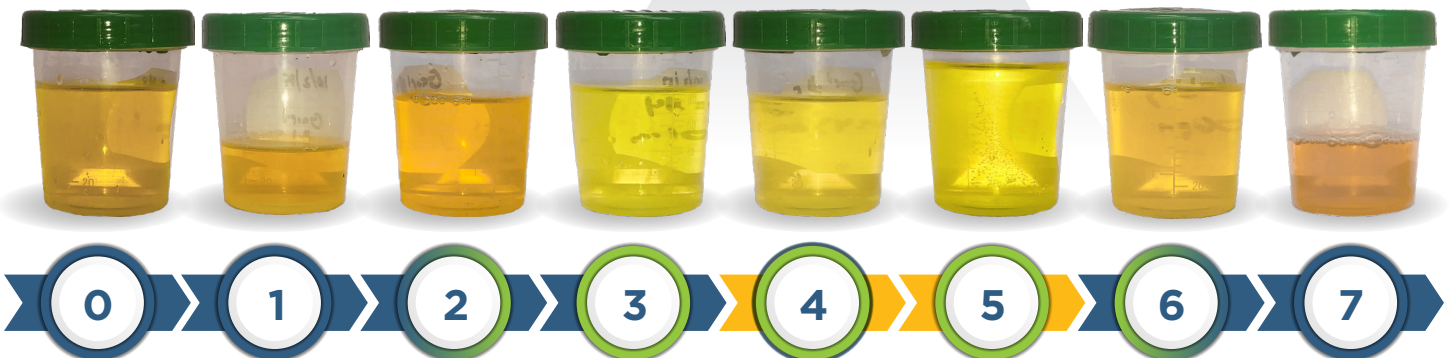

### Here's how they do it

#### MASKING USE INSTRUCTIONS:

1. Drink Rescue Cleanse bottle. Shake well before consuming.
2. Refill half of product bottle with water and consume within 30 minutes.
3. Urinate at least three times.
4. You are now in the clear zone. Urinations 4 & 5 can be presented to the test collector. The clear zone lasts between 2.5 - 5 hours.

### CLEAR ZONE



SPECIMEN	PH	URINE CREAT	SGI	OXH	TRUULD	C/SGR	STANDARD		THC (Cutoff 50)	ETG (Cutoff 1000)	AMP (Cutoff 500)
							SG	UC			
 Normal Sample (8:45am)	6.1	209.6	1.0118	138.4	507.9	2.7	1.025	199.8	157.4	2876.1	542.2
 Sample 1 (9:10am / 25mins)	6.3	198.9	1.0124	194.8	348.6	2.4	1.023	185.5	151.8	2717.1	1007.8
 Sample 2 (9:42am / 57mins)	5.2	79.1	1.0028	65.6	113.7	4.2	1.005	75.4	35.5	1297	943.7
 Sample 3 (9:53am / 68mins)	5.6	25	1.0026	5.5	32.7	1.4	1.003	26.2	0	479.2	510.2
 Sample 4 (10:01am / 76mins)	5.6	20.1	1.0026	3.7	23.7	1.2	1.003	21.4	4.8	268.1	406.7
 Sample 5 (10:43am / 118mins)	5.7	20.8	1.0029	2.9	26.4	1.1	1.003	22.1	-1.5	204.8	347.9
 Sample 6 (11:58am / 193mins)	5.4	140.7	1.0518	41.7	116.4	0.4	1.013	137.5	80.5	1353.3	737.4
 Patient Sample 7 (1:06pm / 261mins)	6.4	164.8	1.0386	62.7	144.3	0.6	1.02	150.3	111.9	1318.1	680